Head C, 100.0 Hz
fs= 500.0 samples per second
dF= 0.0610 Hz
dT= 16.3840 sec

IML-2
Structural Coordinates

MEDS: Life Science Laboratory Equipment

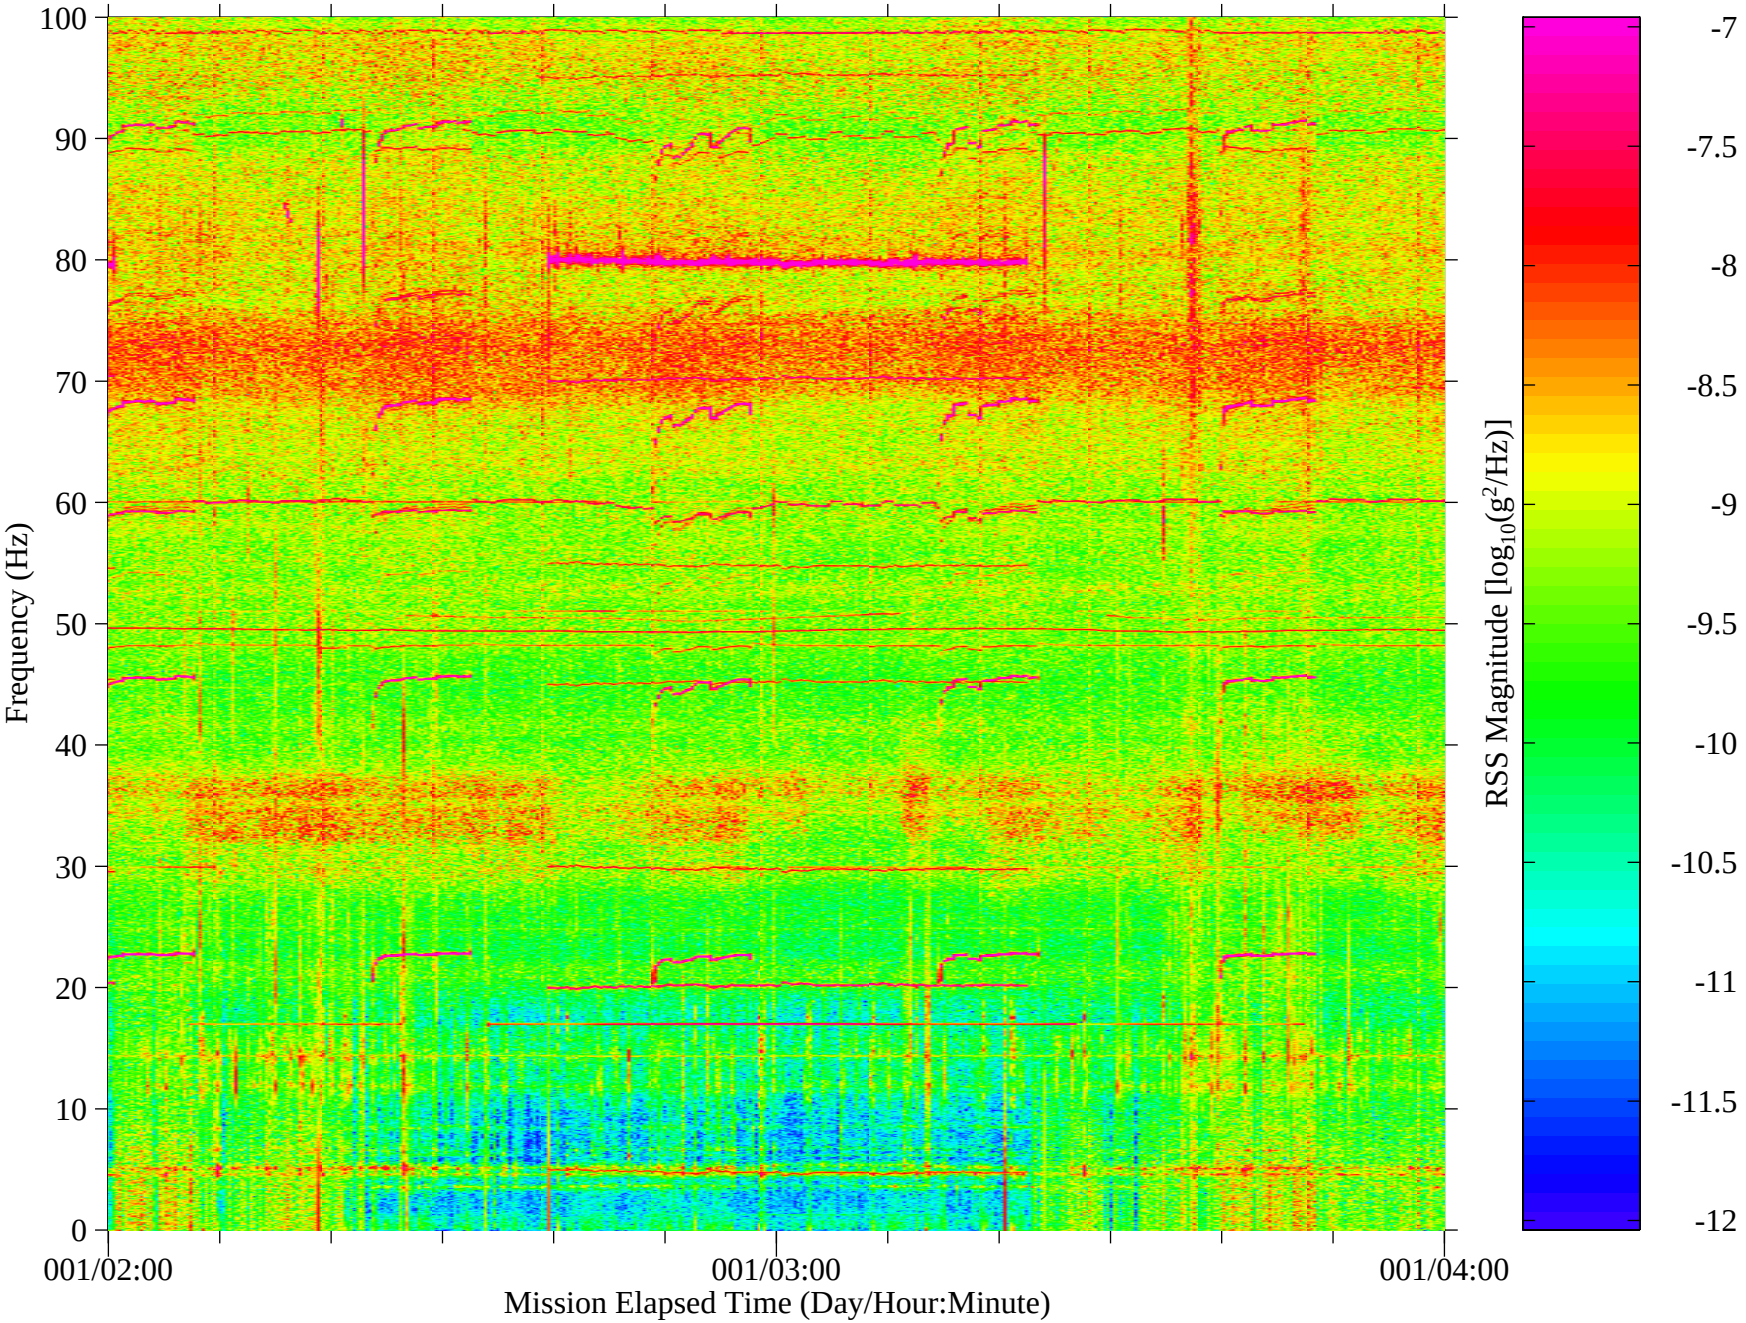

MATLAB: 21-Feb-97, 12:13 pm